

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

MAR 10 2010

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N <u>130303</u> ✓
Name <u>Bon Dudley</u>		ID# <u>3532</u> Date <u>3.15.10</u>
A	Agency <u>Wasilla PD</u>	Phone # <u>352.5408</u>
Instrument Location <u>1900 E. Parks Hwy Wasilla, AK (WPD)</u>		
B	Alco S/N <u>930491</u> ✓	Target Value <u>.083</u> ✓ High Pressure <u>800</u>
Alco Test Value Average <u>.078</u> ✓		<u>.083</u> ✓
1 <sup>st</sup> Alco <u>.078</u>		2 <sup>nd</sup> Alco <u>.083</u>
Signature <u>Bl. Dudley</u> ✓		<u>CRB</u> <u>6/23/10</u>
(OVER)		

(Do Not write in the area below)

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

Nita J. Bolz  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 1<sup>st</sup> day of July 2010.

Carolyn M. Noland (Notary Seal Stamp)

Carolyn M. Noland  
Notary Public, State of Alaska  
Commission Expires with Office



Target value not programmed. Breath

personnel needed to authenticate

VOC for court. CRB 6/22/10

personnel

BT9 03/00

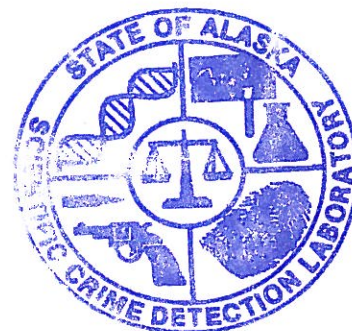

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130303 ✓

(CONTINUED FROM FRONT PAGE)

C

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130303 ✓

MARCH 15, 2010 ✓

OPERATOR'S NAME:

DUDLEY/BEN/H

OPERATOR'S NUMBER: 3532

SUBJECT'S LAST NAME:

VERIFICATION OF CAL

SUBJECT'S FIRST NAME/MI :

L

O.L. #: L

DEPT/AGENCY: WAS1

CASE/REPORT:

TEST TYPE: V

ALCO TARGET VALUE: .083

ALCO S/N: G30491

## --- BREATH ANALYSIS ---

.079 ADJUSTED FOR 29.68 in		
ALCO TARGET	.078	17:26
BLANK TEST	.000	17:27
INTERNAL STANDARD	VERIFIED	17:27
ALCO TV 29.68 in	.083	17:27
BLANK TEST	.000	17:28
SUBJECT SAMPLE	.000	17:28
BLANK TEST	.000	17:29
ALCO TV 29.68 in	.083	17:29
BLANK TEST	.000	17:30

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130303 ✓

MARCH 15, 2010 ✓  
TIME 17:23

## --- DIAGNOSTIC CHECK ---

COMPUTER:	OKAY
PROGRAM:	OKAY
SOFTWARE DATE:	01/08/09
HEATERS	
SAMPLE CHAMBER:	49c
BREATH TUBE:	41c
BAROMETER:	29.68 in
FLOW DETECTOR:	OKAY
PUMP	
HIGH SPEED:	OKAY
DETECTOR:	OKAY
FILTERS:	OKAY
QUARTZ STANDARD:	OKAY
CALIBRATION:	OKAY

## PRINTER TEST

!"#\$%&'()\*+,-./0123456789:;<=>?@ABCDEF  
HIJKLMNOPQRSTUVWXYZ[\]^\_`abcdefghijklmnopqrstuvwxyz  
pqrstuvwxyz{|}~△